

# AQ-SPEC

## Air Quality Sensor Performance Evaluation Center

### Evaluation Summary

#### Sensor Description

Manufacturer/Model:  
Wicked Device/Air  
Quality Egg 2022 Model  
(O<sub>3</sub> & NO<sub>2</sub>)

Pollutant:  
O<sub>3</sub>

Time Resolution:  
1-min



- Overall, the accuracy of the Air Quality Egg 2022 Model sensors ranged from 83.9% to 98.5% and decreased as O<sub>3</sub> conc. increased over the tested concentration range. The sensors underestimated the O<sub>3</sub> measurements from FEM T400 in the laboratory experiments at 20 °C and 40% RH.
- The Air Quality Egg 2022 Model sensors exhibited high precision for all T/RH combinations and all O<sub>3</sub> concentrations.
- The Air Quality Egg 2022 Model sensors (IDs: 233d, 1f4e, 8a60) showed low to moderate intra-model variability in the field and laboratory evaluations.
- Data recovery was ~100% from all units in both field and laboratory evaluations.
- The Air Quality Egg 2022 Model sensors showed very weak to moderate correlations ( $0.20 < R^2 < 0.51$ , 5-min mean) with the corresponding FEM T400 data in the field evaluation and very strong correlations with the FEM T400 in the laboratory evaluations ( $R^2 \sim 0.98$ ).
- The same three Air Quality Egg 2022 Model units were tested both in the field (1<sup>st</sup> stage of testing) and in the laboratory (2<sup>nd</sup> stage of testing).

### Field Evaluation Highlights

- Deployment period 03/18/2022 to 05/18/2022 : the three Air Quality Egg 2022 Model sensors showed very weak to moderate correlations with the corresponding FEM O<sub>3</sub> data.
- The units exhibited low intra-model variability and data recovery for O<sub>3</sub> measurements was ~100% from all units.

#### Additional

##### Field evaluation report:

<http://www.aqmd.gov/aq-spec/evaluations/criteria-pollutants/field>



##### Lab evaluation report:

<http://www.aqmd.gov/aq-spec/evaluations/criteria-pollutants/laboratory>

##### AQ-SPEC website:

<http://www.aqmd.gov/aq-spec>

5-min mean  
 $0.20 < R^2 < 0.51$

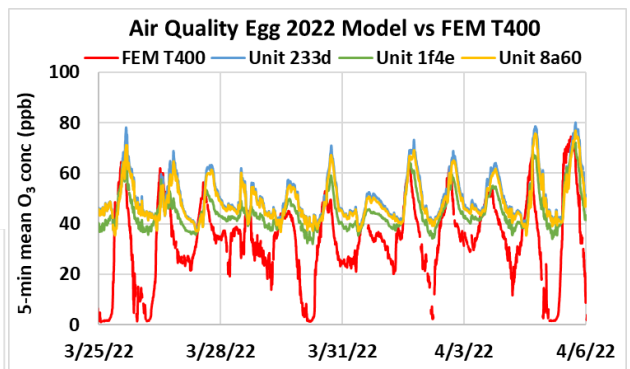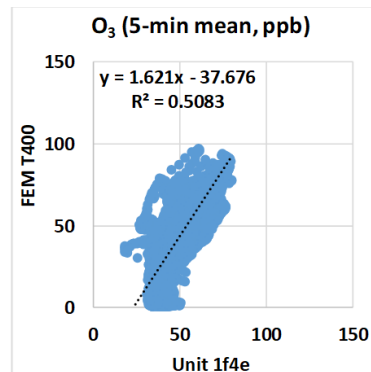

Coefficient of Determination ( $R^2$ ) quantifies how the three sensors followed the O<sub>3</sub> concentration change by the reference instruments.

An  $R^2$  approaching the value of 1 reflects a near perfect agreement, whereas a value of 0 indicates a complete lack of correlation.

# Laboratory Evaluation Highlights

## Accuracy (O<sub>3</sub>)

$$A (\%) = 100 - \frac{|\bar{X} - \bar{R}|}{\bar{R}} * 100$$


Steady State (#)	Sensor Mean (ppb)	FEM T400 (ppb)	Accuracy (%)
1	28.9	28.5	98.5
2	45.0	47.5	94.8
3	76.0	88.6	85.7
4	126.4	150.6	83.9
5	215.6	257.0	83.9

Accuracy was evaluated by a concentration ramping experiment at 20 °C and 40% RH. The sensor's readings at each ramping steady state are compared to the reference instrument.

A negative % means sensors' overestimation by more than two fold. The higher the positive value (close to 100%), the higher the sensor's accuracy.




## Precision (O<sub>3</sub>)

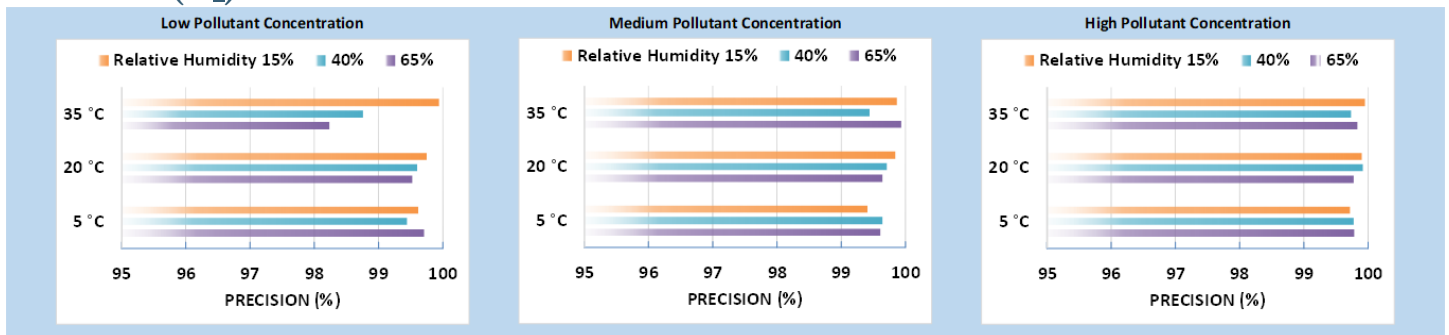

100% represents high precision.

Sensor's ability to generate precise measurements of O<sub>3</sub> concentration at low, medium, and high pollutant levels were evaluated under 9 combinations of T and RH, including extreme weather conditions like cold and dry (5 °C and 15% RH) cold and humid (5 °C and 65% RH), hot and humid (35 °C and 65% RH), or hot and dry (35 °C and 15% RH).

## Coefficient of Determination

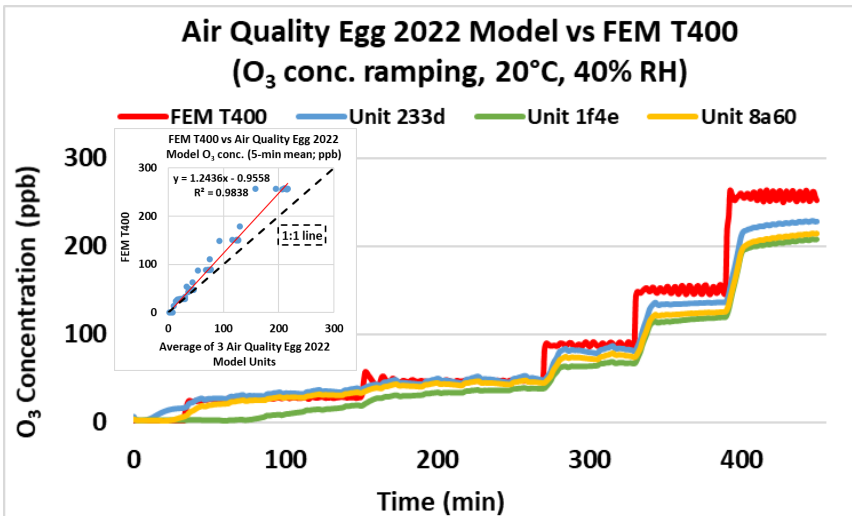

The Air Quality Egg 2022 Model sensors showed very strong correlations with the corresponding FEM T400 O<sub>3</sub> data (R<sup>2</sup> ~0.98) at 20 °C and 40% RH.

## Climate Susceptibility

From the laboratory studies, temperature and relative humidity had minimal effect on the precision of the Air Quality Egg 2022 Model sensors' ozone measurements.

## Observed Interferents

NO<sub>2</sub>



All documents, reports, data, and other information provided in this document are for informational use only. Mention of trade names or commercial products does not constitute endorsement or recommendation. As a Government Agency, the South Coast AQMD and its AQ-SPEC program highly recommend interested entities to make use and purchase decisions based on the requirements of their study design, the technical aspects and features of their specific project applications.